


VISION COVID-19 SALIVA AG RAPID CE IVD TEST KIT

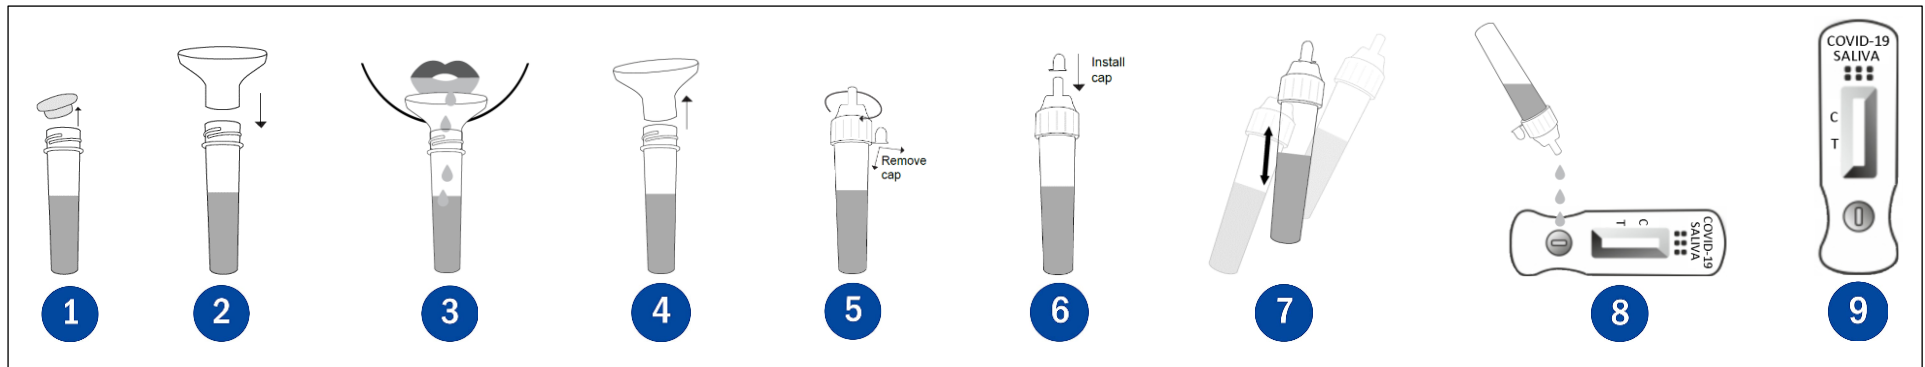

1. Uncap the reagent tube
2. Install
3. 500 µl, fill line
4. Unscrew the lid

5. Close the vial
6. Instal cap
7. Shake the vial for 5 secs.
Wait 1 min. to let the sample


- dissolve in the extraction reagent
8. Put 2 drops into sample well
9. Wait 10-15 mins. Observe the result



Positive



Negative



Invalid